

### Information pest: *Candidatus phytoplasma vitis* and *Candidatus phytoplasma solani*

Flavescence dorée (FD) is one of the greatest threats for grapevine in Europe. It is caused by the phytoplasma *Candidatus phytoplasma vitis*, belonging to the elm yellows group (16SrV group), efficiently transmitted by the vector *Scaphoidus titanus*. This phytoplasma is a regulated plant pathogen in Europe and is included in European legislation as a quarantine pest.

Bois noir (BN) is caused by the phytoplasma *Candidatus phytoplasma solani*, belonging to the 16SrXII-A group, transmitted principally by the vector *Hyalesthes obsoletus*.

Disease symptoms develop mainly in summer. Leaves turn yellow or red depending on the cultivar. They roll down-ward and become brittle; the interveinal area of leaves may become necrotic. Shoots show incomplete lignification.

Flavescence dorée's symptoms are similar to those caused by other yellows diseases of grapevine, in particular Bois noir; molecular diagnostic is the only way to differentiate these two phytoplasmas.

### Introduction

The PCR FD BN kit has been developed by QualiPlante according to the previous French official method MOA006A-1b: "*détection des phytoplasmes de la vigne du groupe 16SrV (flavescence dorée) et du groupe 16SrXII (bois noir) – PCR multiplex gigogne*", currently replaced by a Real-Time PCR method. This method was evaluated during the EUPHRESKO Grafdepi I project (results available from [www.euphresco.net/media/project/reports/grafdepi\\_final\\_report.pdf](http://www.euphresco.net/media/project/reports/grafdepi_final_report.pdf)).

This Duplex Nested End-Point PCR method includes for the 1<sup>st</sup> amplification specific primer sets for the detection of each phytoplasma groups (FD9f/FD9r and STOL11f2/STOL11r1) and for the 2<sup>nd</sup> amplification specific primer sets for each of the phytoplasma groups searched with specific sequences for the 1<sup>st</sup> PCR product (FD9r2/FD9f3b and STOL11f3/STOL11r2).

*This product should be used only for research purposes.*

### Intended use

The PCR kit is validated for the simultaneous detection of Flavescence dorée and Bois noir in Duplex Nested End-Point PCR. Suitable tissues are grapevine leaves, preferably primary veins and petioles and bark scrapings from dormant canes.

It is preferable to test plant tissues with vine yellows symptoms.

### Kit format and content

Two kits are available for 24 and 96 tests.

Article N°	Product name
nPCR FDBN 24	Nested PCR Flavescence dorée/Bois noir 24 tests
nPCR FDBN 96	Nested PCR Flavescence dorée/Bois noir 96 tests

Content	24 tests	96 tests
Direct Master Mix	24 tests	2x48 tests
Nested Master Mix	24 tests	2x48 tests
Positive Control	3 tests	8 tests
Negative Control	3 tests	8 tests

### Storage conditions

This kit can be shipped at room temperature but upon receipt it should be stored immediately at the recommended storage temperature: **from -30 ° C to -10 ° C**.

Avoid prolonged exposure to light and repeated freeze and thaw cycles.

### Shelf life

If the kit is correctly stored, at constant-temperature freezer, its performance is guaranteed until the expiration date indicated on the tubes label.

### Materials and equipment (not provided)

- DNA extraction tools and reagents
- Nuclease-free filter tips and micropipettes
- Optical grade nuclease-free tubes/plate
- Disposable latex or vinyl gloves
- DNA ladder and loading-dye buffer
- PCR thermal cycler
- Agarose gel reagents and apparatus

### Nucleic acids extraction

Extract DNA from samples according to your usual protocol. Upon request, QualiPlante can recommend you an extraction method.

## FIRST PCR

### Reaction set-up

- Slowly thaw **Direct Master Mix** by placing it on ice or at 4°C.
- Shake briefly **Direct Master Mix** and spin down the liquid.
- Add 20 µl of **Direct Master Mix** (without DNA template) to each PCR tubes or wells of an optical-grade PCR plate.
- Add 2 µl of DNA template to the **Direct Master Mix**. Do not forget to prepare a PCR tube or well of a PCR plate for the **Positive Control** and the **Negative Control**.

Components	Volume/PCR tube or well
DNA template or <b>Positive control</b> or <b>Negative control</b>	2 µl
<b>Direct Master Mix</b>	20 µl
Total Volume / PCR tube or well	22 µl

In order to confirm the absence of any reagent's contamination, we strongly recommend including a no-template control (e.g. DEPC water) in the assay.

### Run and thermal cycling

- Seal carefully the PCR tubes or PCR plate. Centrifuge briefly to collect components at the bottom of the PCR tubes or wells of the plate. Protect from light before thermocycling.
- Load the PCR tubes or plate into the PCR thermal cycler and follow the thermal cycling below:

Steps	Temp (°C)	Time	Cycle(s)
Initial denaturation	94°C	3 min	1
Denaturation	94°C	1 min	35
Annealing	55°C	1 min	
Elongation	72°C	1 min 30 sec	
Final elongation	72°C	10 min	1
Storage	4°C	∞	-

### Dilution of 1<sup>st</sup> PCR products

Using DNase and RNase free PCR tubes, **dilute to 1:1.000** in sterile water each PCR product for samples, **Positive Control** and **Negative Control** obtained during the previous step.

Shake and spin down each tube.

## SECOND PCR

### Reaction set-up

- Slowly thaw **Nested Master Mix** by placing it on ice or at 4°C.
- Shake briefly **Nested Master Mix** and spin down the liquid.
- Add 20 µl of **Nested Master Mix** (without DNA template) to each PCR tubes or wells of an optical-grade PCR plate.
- Add 5 µl of **diluted PCR products** to the **Nested Master Mix**. Do not forget to prepare a PCR tube or well of a PCR plate for the PCR products obtained with **Positive Control** and **Negative Control**.

Components	Volume/PCR tube or well
PCR products from the 1 <sup>st</sup> PCR diluted to 1:1.000 (*)	5 µl
<b>Nested Master Mix</b>	20 µl
Total Volume / PCR tube or well	25 µl

(\*) See the section "Dilution of 1<sup>st</sup> PCR products"

### Run and thermal cycling

- Seal carefully the PCR tubes or PCR plate. Centrifuge briefly to collect components at the bottom of the PCR tubes or wells of the plate. Protect from light before thermocycling.
- Load the PCR tubes or plate into the PCR thermal cycler and follow the thermal cycling below:

Steps	Temp (°C)	Time	Cycle(s)
Initial denaturation	94°C	3 min	1
Denaturation	94°C	1 min	35
Annealing	56°C	1 min	
Elongation	72°C	1 min 30 sec	
Final elongation	72°C	10 min	1
Storage	4°C	∞	-

### Agarose gel electrophoresis

Prepare an agarose gel at 1% w/v in 1X-TAE buffer.

#### Gel loading:

- load the DNA ladder (for example 100-2'000 bp DNA step ladder).
- load 10 µl of the PCR products from the previous step adding the loading dye buffer (not provided in the kit).

**Run:** run the gel electrophoresis for 40-45 minutes at 80V.

## Results analysis


### ANALYSIS VALIDATION

Flavescence dorée is detected when a **1.160 bp** DNA fragment is observed. Bois noir is detected when a **720 bp** fragment is observed.

The analysis is validated when:

- ✓ 2 DNA fragments, one of 1.160 bp and one of 720 bp, are visible in the positive control lane.
- ✓ no DNA fragment is visible in the negative control lane.

The picture below represents a 1X-TAE 1% agarose gel showing the DNA amplification of Flavescence dorée and Bois noir in grapevine:

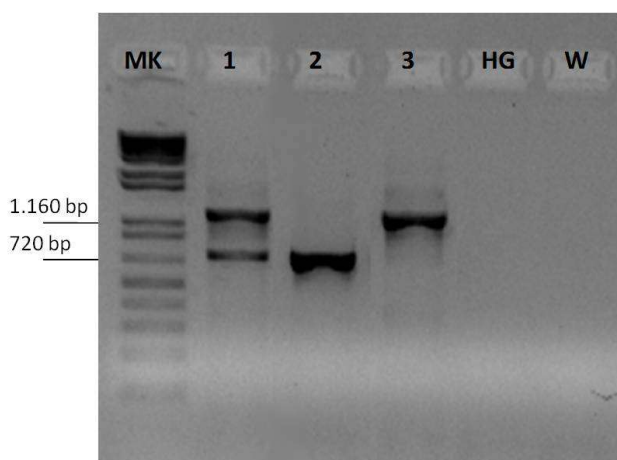

**MK:** DNA ladder - **1:** Positive Control or sample infected by FD and BN - **2:** Sample infected by BN - **3:** Sample infected by FD - **HG:** Negative Control or healthy sample - **W:** No template control

### RESULTS INTERPRETATION

The specific product of Flavescence dorée is a **1.160 bp** DNA fragment. The specific product of Bois noir is a **720 bp** fragment.

- ✓ A sample is infected by Flavescence dorée if a 1.160 bp specific fragment is present in the PCR reaction.
- ✓ A sample is infected by Bois noir if a 720 bp specific fragment is present in the PCR reaction.
- ✓ A sample is infected by Flavescence dorée and Bois noir if 2 DNA fragments, one of 1.160 bp and one of 720 bp, are present in the PCR reaction.
- ✓ A sample is not infected by Flavescence dorée and Bois noir if none DNA fragment is present in the PCR reaction.

The table below summarizes the results interpretation:

Fragment size		Interpretation	
1.160 bp	720 bp	FD	BN
-	-	Negative	Negative
✓		<b>POSITIVE</b>	Negative
✓	✓	<b>POSITIVE</b>	<b>POSITIVE</b>
	✓	Negative	<b>POSITIVE</b>

### Special handling instructions

This kit was designed to be used by laboratory staff trained to follow the usual molecular biology precautions. Always perform the tests in a nuclease-free work environment. Always wear gloves when handling samples containing DNA and the components of the kit. Do not touch any kit components with an ungloved hand. Use appropriate laboratory disposable parts. Use nuclease-free tubes and filter tips to avoid degradation and cross-contamination. Do not use components from kits with different batch numbers in the same test procedure. Do not interchange reagents with other kits. To avoid cross-contamination, use separate rooms for (a) nucleic acids extraction, (b) preparation of the Master Mix and (c) amplification. To avoid cross-contamination and obtain reliable results, it is essential to strictly follow the protocol in this manual. Avoid unnecessary freeze-thaw cycles of the kit components. Do not use reagents after their expiration date.

### Troubleshooting

Post-PCR data analysis shows no amplification, or amplification plots look grossly abnormal:

Possible causes	Corrective actions
Evaporation of the sample due to inadequate sealing of the plate	Repeat the test using the appropriate tools to seal correctly the plate
Consumables are not appropriate for the method	Repeat the test using consumables recommended by the thermal cycler supplier
The quality of nucleic acid extracted is low	Repeat the extraction step. Ensure that the method of extraction has been performed correctly. In any doubt, please, contact us
Abnormal amplification	Centrifuge the plate briefly to spin down the contents and eliminate any air bubbles

**No amplification reaction is observed in the positive control well, while other samples are positive:**

Possible causes	Corrective actions
The positive control provided with the kit was not added into the reaction well	Repeat the test. If the problem persists, please, contact us

**An amplification plot is observed in the negative control well:**

Possible causes	Corrective actions
Contamination of the negative control or the Master Mix with target-positive nucleic acid	Repeat the test by applying appropriate quality procedures to prevent contamination. Seal the plate correctly

## Warranty and Responsibilities

Qualiplante SAS guarantees the buyer exclusively concerning the quality of reagents and of the components used to produce the Kits. Any product not fulfilling the specifications included in the product sheet will be replaced. This warranty limits Qualiplante SAS responsibility to the replacement of the product. No other warranties, of any kind, express or implied-are provided by Qualiplante SAS.

Qualiplante SAS is not responsible and cannot anyway be considered responsible or jointly responsible for possible direct and indirect damages resulting of the use and/or the misuses of the Kits. The user consciously and under her/his own responsibilities decides for the utilization purposes of the Kits and uses it the way she/he considers most suitable in order to reach her/his goals and/or objectives. Qualiplante SAS is not responsible for the data resulting from the use of the Kits, for the utilization that the user independently decides to make of them or for the direct or indirect damages possibly resulting from the disclosure or transmission of the data themselves to third parties under any form or circumstance. This clause is automatically accepted by the user when purchasing the Kits.

Some of the applications which may be performed with this product may be covered by applicable patents in certain countries. The purchase of this product does not include or provide a license to perform patented applications. Users may be required to obtain a license depending on the country and/or application. Qualiplante SAS does not encourage the unlicensed use of patented applications. The Kits may require the use of Taq Polymerase enzyme, DNA binding components and fluorochromes/quencher, often registered as trademark by companies. The product, equipment and information included in the Kits consist of assembled reagents. The Kits are designed for the services supply, quality control or any other application that is not exclusively an internal company's research and requires a specific license for PCR and Real-Time PCR use. The license and authorization for PCR and Real-Time PCR use are not included in the Kits. The user is responsible for setting prefixed goals, choosing whether or not to perform the PCR or Real-Time PCR reaction and to apply for register her/his own license.

The Kits have been internally tested by our quality control. Any responsibility is waived if the warranty of quality control does not refer to the specific Kits. The user is personally responsible for data that she/he will obtain and/or she/he will supply to third parties using these Kits. Once the sealed package is opened the user accepts all the conditions without fail; if the package is still sealed the kit can be returned and the user can be refunded.

Kits components are intended, developed, designed, and sold for Research Purpose Only. Product claims are subject to change.